

Research Space

Journal article

4D Printing of origami structures for minimally invasive surgeries using functional scaffold

Langford, T, Mohammed, A., Essa, K., Elshaer, A. and Hassanin, H.

4D Printing of Origami Structures for Minimally Invasive Surgeries of Functional Scaffold

Thomas Langford ¹, Abdullah Mohammed ², Khamis Essa ², Amr Elshaer ³, and Hany Hassanin ⁴

1 School of Engineering, University of Liverpool, Liverpool, L69 3BX, UK

2 School of Engineering, University of Birmingham, Birmingham, UK

3 Drug Discovery, Delivery and Patient Care (DDNPC), School of Life Sciences, Pharmacy and Chemistry, Kingston University London, Kingston Upon Thames, Surrey, KT1 2EE, UK

4 School of Engineering, Technology, and Design, Canterbury Christ Church University, Canterbury, CT1 1QU, UK

Corresponding author: Hany Hassanin hany.hassanin@canterbury.com

The authors declare no conflict of interest

Abstract

Origami structures have attracted attention in biomedical applications due to their ability to develop surgical tools that can be expanded from a minimal volume to a larger and functional device. On the other hand, Four-dimensional (4D) printing is an emerging technology, which involves 3D printing of smart materials that can respond to external stimuli such as heat. This short communication introduces the proof of concept of merging origami and 4D printing technologies to develop minimally invasive delivery of functional biomedical scaffolds with high shape recovery. The shape memory effect (SME) of the PLA filament and the origami designs were also assessed in terms of deformability and recovery rate. The results showed that herringbone tessellation origami structure combined with internal natural cancellous bone core satisfies the design requirement of foldable scaffolds. The substantial and consistent SME of the 4D printed herringbone tessellation origami that exhibited 96% recovery compared to 61% for PLA filament was the most significant discovery of this paper. The experiments demonstrated how the use of 4D printing in situ with origami structures could achieve reliable and repeatable results. Therefore, conclusively proving how 4D printing of origami structures can be applied to biomedical scaffolds.

Keywords: Origami; Additive Manufacturing; 4D printing; Scaffolds; shape memory

polymer

1. Introduction

Bone is a complex structure that is made up of several constituents such as fibres, cells, and minerals. This structure is far different from other human tissues; the extracellular cells are mineralised, which give it significant mechanical strength and stiffness. As a result, it plays a significant role to support the body structure and allows the movement of Skelton ^[1]. Several medical problems can lead to the loss or the damage of human bones such as disease, trauma and injury, which requires medical treatment. Bone repair, regeneration or replacements focuses on tissue replacement from human body site to another, autograft, or from one person to another, allograft. Although these procedures have been well established and have shown excellent results, major issues are in both techniques such as being painfully expensive, constrained, and subject to infection or body rejection in case of an allograft ^[2]. Bone scaffolds represent a favourable alternative to autograft and allograft techniques. They are used as a template for cell attachment, proliferation, and differentiation to promote bone regeneration. Bone scaffolds require being biocompatible, biodegradable, strong, and porous to promote the flow of body fluid ^[3, 4]. However, placing current scaffolds designs can require highly invasive surgery, which is often required so that there is space to place what can be large and bulky scaffolds. Scaffold insertion can be particularly damaging to the patient depending on where it is being placed. Minimally invasive surgery is associated with fewer complications, less pain, shorter hospital stay, as well as the cosmetic benefit of reducing post-surgery scars. Implementing minimally invasive surgery in bone scaffolds treatment requires smart scaffold that can be deformed before insertion and then recovery it once in position so that it would mean smaller points of incision would be required.

Additive manufacturing (AM) or 3D printing is the manufacturing of a 3D object layer by layer from a digital design. There are several categories of AM technologies such as Powder bed

fusion, Material Extrusion, Direct Energy Deposition, Vat Photo Polymerisation, Binder Jetting, Sheet lamination, and Material Jetting. Material extrusion is a low cost, easy to use and available technique in many commercial forms ^[5, 6]. In Material extrusion, the material is extruded under pressure through a nozzle according to a digital design. The extruded material is deposited on top of each layer and solidify. Fused deposition modelling (FDM) is a technique of material extrusion where a thermoplastic filament is softened by heaters and extruded from a nozzle, whereas, pneumatic or syringe extrusion (PE/SE) techniques extrude paste materials such as ceramic clays. Vat polymerisation (VP) technique uses UV to initiate the cross-linking of a layer of photosensitive resin to cure it into a solid polymer. Afterwards, another layer of the polymer is deposited and cured onto the past layers until the part is completed. VP techniques include stereolithography (SLA), continuous liquid interface production (CLIP), digital light processing (DLP), and photon polymerisation ^[7-10]. The technique has been adopted to fabricate polymer and ceramic micro parts for MEMS applications as it outperformed the conventional soft lithography processes that are limited to fabricate 2.5 D parts and not real 3D components ^[11-17]. Powder bed fusion (PBF) is an approach at which a laser beam selectively scan a layer of the powder according to a digital design to build components in the typical layer-wise way ^[18, 19]. In direct energy deposition (DED), a laser or electron beam is focused on melting metal powder. The molten droplets are then deposited on the top of a substrate. Laser energy net shaping (LENS), Laser deposition welding (LDW), and wire and Arc AM (WAAM) are widely used techniques of DED ^[20-22]. In binder jetting, the powder is bound by spraying binder droplets from a jet on a top of a layer of powder then the powder platform is then lowered to apply another layer on top of the first layer ^[23-25]. Sheet lamination (SL) cuts and glues layers of materials by using a laser beam, or ultrasonic to bond the stacked layers. Additional machining and surface finishing are typically used after 3D printing ^[26, 27]. In material Jetting (MJ), droplets of the materials are deposited and dried or

cured layer by layer. They are different ways to deposit the material such as in continuous inkjet at which the material is deposited with the aid of continuous pressure ^[28, 29], and drop on demand (DOD) which uses discrete pressure instead of continuous pressure ^[30]. Additive manufacturing has the ability to process a wide range of materials such as metals ^[31], polymers ^[32], and ceramics ^[4]. The technology has been adopted in many industries, such as aerospace ^[33, 34], biomedical ^[35], defence ^[36], energy ^[37]. Four-dimensional (4D) printing is an emerging technology that refers to the additive manufacture of material that responds to changes in its immediate environment. Therefore, enabling engineered solutions to be recovered without direct human or computer interaction. The technology was first introduced in 2013 and since then attracts great attention in many biomedical applications. 4D printing offers several benefits such as the ability to produce smart products from smart material, change of product geometry when required, and adding innovation in the design and development stage ^[36]. These benefits enabled the penetration of this technology to broad applications in engineering, dentistry, medical, and material science.

Shape-memory polymers are stimuli-responsive polymers that can change their shape from one to another by the use of heat, light, or electricity. The thermally induced shape memory effect presents in specific polymers is due to shape recovery of polymers when subject to heat. The chains in the amorphous polymers are completely dispersed randomly in the matrix without the restriction of crystallites in semicrystalline polymers. On the other hand, movements of the polymer segments are frozen in the case of the glassy state. The rubber-elastic state starts when increasing the activation energy, which initiates the rotation around the segment bonds. This enables the polymers chains to take up energetically equivalent shapes with compact random macromolecules. The rubbery state occurs above the glass transition temperature (T_g), and the polymer becomes flexible. The original shape of the polymer can be recovered when it is

plastically deformed only upon heating to above T_g . In this case, physical or chemical cross-link works to store the elastic energy during shape programming and the driving recovery force [38]. The presence of shape-switching parts nodes or shape-fixing parts in polylactic polymers PLAs is behind the shape recovery. Both physical cross-links and the crystallisation of PLAs act as the net-points and therefore have the shape-memory ability. However, the shape-memory effect of PLA polymers is often restricted to minor deformations it breaks when programming PLA with more than 10%. This limits the potential for using PLA for minimally invasive surgeries [39].

This communication introduces a design and manufacturing approach to develop deployable scaffolds using 4D printing of shape memory polymer (SMP) that will be inserted into a cavity in the body through minimally invasive surgery. Once in position, the scaffold will be recovered, causing it to increase in size and fill the cavity where it will substitute as the tissue's extracellular matrix (ECM). The ECM coordinates how cells coordinate with each other as well as providing overall structure to a tissue. An engineered tissue scaffold replicates a diseased or damaged tissue's ECM temporarily when a native ECM is not present. Scaffolds are used to aid the recovery of a patient when a cavity in the tissue would prohibit the normal regeneration of the tissue. Therefore, a scaffold will be inserted into a cavity to substitute as the ECM so that healthy cells may migrate and proliferate across it, filling the cavity. The primary focus of this paper was not on the biomedical interaction between cells and the scaffold but was instead focused on achieving the benefit of SMP and smart structures in tissue engineering and to introduce the proof of concept of deployable biomedical scaffolds using origami structures.

2. Design and Experimental

There are multiple types of additive manufacture and processed materials. However, this study employs FDM as it the most common method to process polylactic acid (PLA). PLA lends

itself particularly well to medical applications since it is biodegradable, biocompatible, non-toxic, and an eco-friendly polymer ^[40]. Therefore, it has full clearance to be used as a material for medical implants by both the European Medical Agency (EMA) and the Federal Drug Administration (FDA). In addition to its ability to be used for implants, it is a shape memory polymer (SMP) meaning PLA can be 4D printed.

2.1 Origami Design

Origami tessellations are origami-folding patterns that repeat themselves and therefore can be scaled up and down depending on application with the potential of the fold being infinitely repeated. Different tessellations enabled for acute management of pre-and post-shape recovery as well as how the polymer would origami move between the states ^[41, 42]. The design of the scaffolds was split into microstructure and macrostructure design. The microstructure design was concerned with how the scaffold's pores are shaped, sized, and arranged to promote cell differentiation, migration, and proliferation. Whereas, the macrostructure was concerned with the design of a recovered scaffold. The primary consideration of the macrostructure was to replicate bone morphology while simultaneously employing origami techniques to exploit the SME of PLA.

Origami Herringbone and Waterbomb tessellation designs were considered in this study as shown in Figure 1a,b. The tessellations were curved around on itself to create a tube. As recovery occurs, the cavity in the middle grows and so accurately represents the medullary cavity found in many long bones. By far the most significant benefit of this design is the substantial difference in volume between recovered and collapsed forms Figure 1c shows how compressing, what is already very similar in structure to real cancellous bone, will close the gaps between replicated trabeculae, allowing for a smaller geometry before recovery. Almost all bones have a section of compact bone with a cancellous bone interior. Therefore, this kind

of scaffold would be highly transferable between different bones within the body. There are two potential problems with this design. First, the size difference between deformed and recovered form is not as significant as in other designs. Secondly, and most importantly, this design does not offer a great solution to reducing the size of the scaffold that needs to substitute for compact bone. The combination of an origami design for the outer edges of the scaffold, which would substitute for compact bone, and the porous replica of cancellous bone to fill the centre, as shown in Figure 1d. This merger of designs eliminates the weaknesses of the individual designs to create a solution that will meet the needs of the patient, and surgeon.

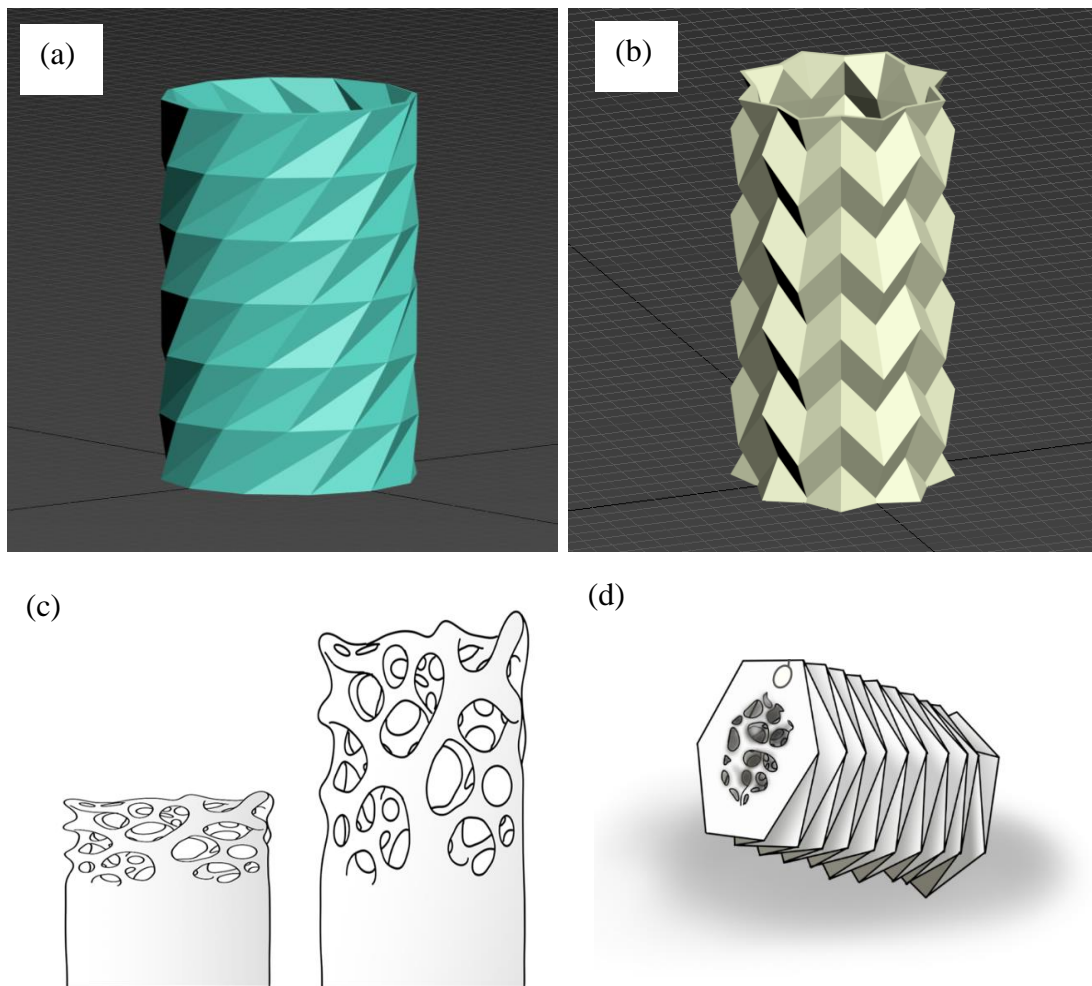


Figure 1. CAD drawing of (a) herringbone tessellation origami, (b) Waterbomb tessellation origami, (c) Natural cancellous bone, (d) Combined tessellation origami and natural cancellous bone design

2.2 Fabrication and Characterisation

The as-received PLA filaments (PLA, makerbot-UK) were tested first using a standard dynamic-mechanical analyser (DMA, Kingston University) to investigate the effect of the heating temperature on the storage modulus. Dynamic mechanical analysis (DMA) was generally used to assess polymers viscoelastic properties as they change from glassy to rubbery like characteristics. Filaments with 0.7 mm in diameter were cut to a length of 15 cm and attached to the dynamic-mechanical analyser at a frequency of 1 Hz and heated from 25 to 90 °C.

Two properties are associated with shape memory polymers. These are the shape fixity and shape recovery. Shape fixity is the ability of the switching points to fix the temporary shape, whereas shape recovery measures the ability of SMP to recover their original shape. Many SMPs such as PLA have high shape fixity but poor shape recovery, as the material can not generate sufficient recovery force during. We focus on this research to measure the shape recovery of PLA filament to understand the material characteristics independently of the design influence. 1.75mm diameter PLA filament was cut into 30x straight test samples of 100mm length. Samples were placed in the slit in threes and heated to the melt temperature of 200°C. Due to all polymer cross-links breaking at this temperature, the samples straightened out under their weight. Once removed and allowed to cool samples were ready for the experiment. Samples were heated to just above the T_g of approximately 60°C-65°C in a water bath of 70°C, shown in figure 24. The reason for using a water bath with a temperature higher than the T_g was so tested samples would not fall below the glass transition temperature when they were taken out of the water for deformation. Samples were taken out individually and deformed to a range of predetermined angles and allowed to cool. Once cooled back to room temperature, each sample angle was remeasured because it was common that the angle achieved was a few

degrees off the intended angle. Samples were then re-submerged in the water bath at 70°C, and the shape memory effect was observed. After only a few seconds, the samples would start returning to their original programmed straight form. Within no more than 10 seconds, the shape memory effect was over. Once the SME was complete, the samples could cool. The recovery angle of each sample was measured. The difference between the recovered angle and the actual test angle was calculated as a percentage of the actual test angle. This percentage shows how much the geometry recovered. Figure 2 shows the experimental procedure of measurement of shape memory effect of PLA filaments.

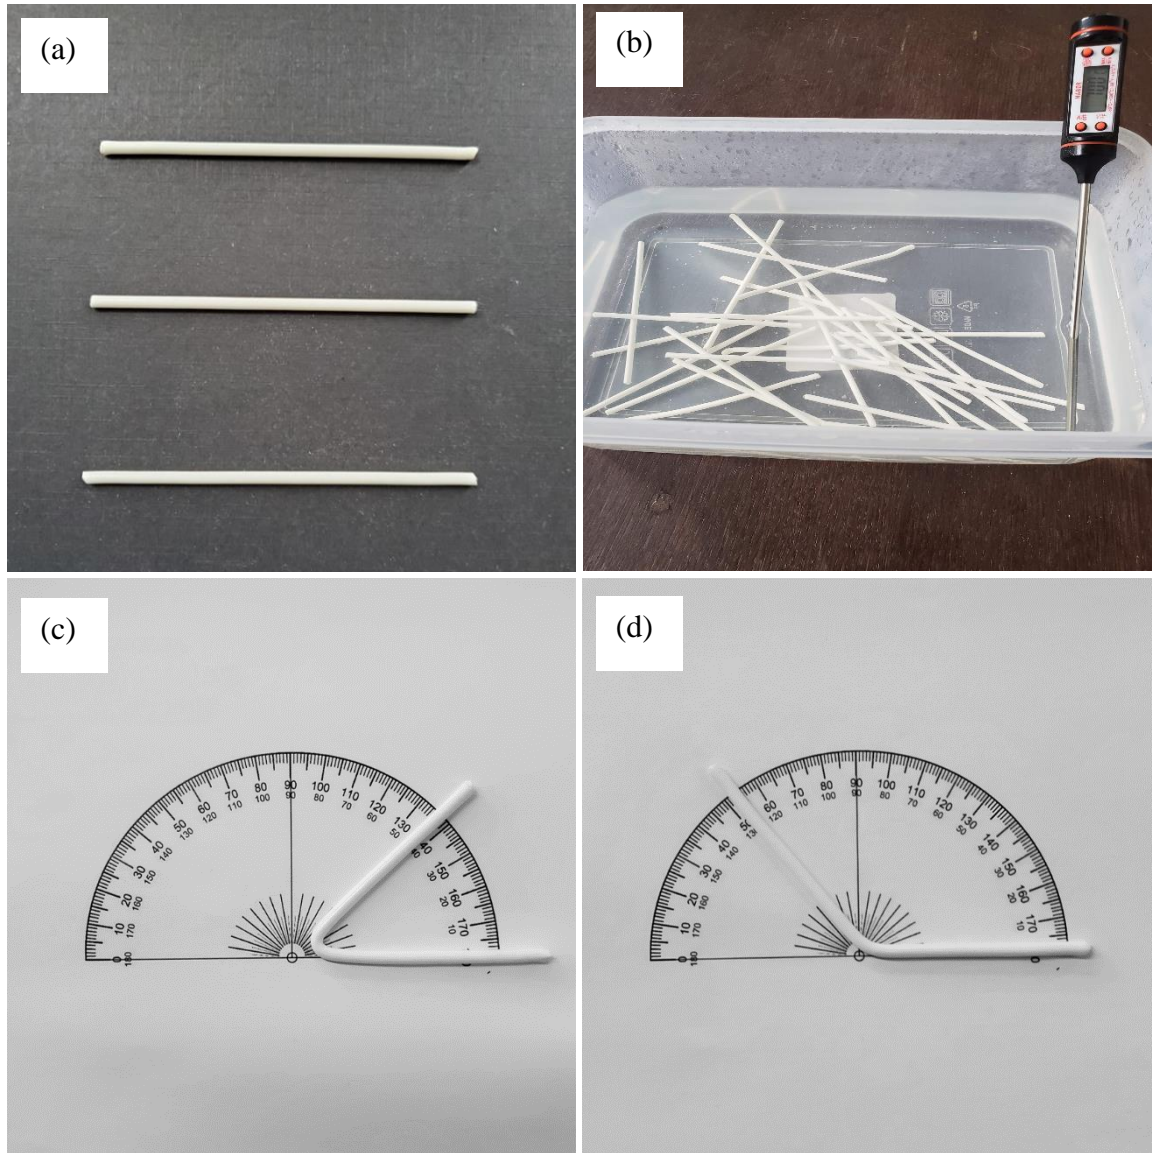


Figure 2: (a) Preparing PLA samples, (b) 70°C Water bath heating test samples; (c) one of the samples deformed shape (d) recovered shape.

The tubular and the modified herringbone tessellation origami structures were 3D printed using makerbot replicator 2. PLA 1.75 mm filament was used as the feeding stock in the 3D printer. The objects were printed with 0.15mm layer thickness at 100mm in height, 60mm in diameter and with a 2.5mm wall thickness, from PLA to produce the prototypes. Similarly to the SME measurements of the PLA filament, The models were characterised in terms of the deformation and recovery to test how the SME would affect the behaviour of the two origami models. The

aim was to realise the most significant and consistent SME possible, but this time within the whole models. Another aspect of the experiment was whether the 61.5% recovery found in PLA filament was a reproducible percentage recovery figure for origami folds.

The printed objects were subject a compressive force and twisted torque causing deformation under to just above the T_g of approximately 60°C-65°C in a water bath at 70°C. The reason for using a water bath with a temperature higher than the T_g was so tested samples would not fall below the T_g when they were taken out of the water for deformation. The prototypes were removed one at a time from the water bath and deformed. Twisted torque and compression load with the aid of a G-clamp were used because they meant that the load could be kept on the prototypes as they were allowed to cool. The deformation amount was determined by when the folds had fully folded in on themselves. Once cooled back to room temperature, each deformed prototype was measured to calculate the ratio between initial print size and deformation size. Samples were then re-submerged in the water bath at 70°C, and the shape memory effect was observed. Once the SME was complete, the samples were removed from the bath and allowed to cool. The difference between the recovered geometry and the deformed geometry was calculated as a percentage of the deformed geometry.

3. Results and Discussion

3.1 Dynamic Mechanical Thermal Properties of the PLA filaments

Figure 3 shows the dynamic mechanical thermal properties of the PLA filaments when heated from 25 to 90 Celsius. The as received filaments show a near plateau storage modulus over temperature range from 30 to 65 Celsius at which it drops sharply afterwards where it changes from the glassy to the rubbery state.

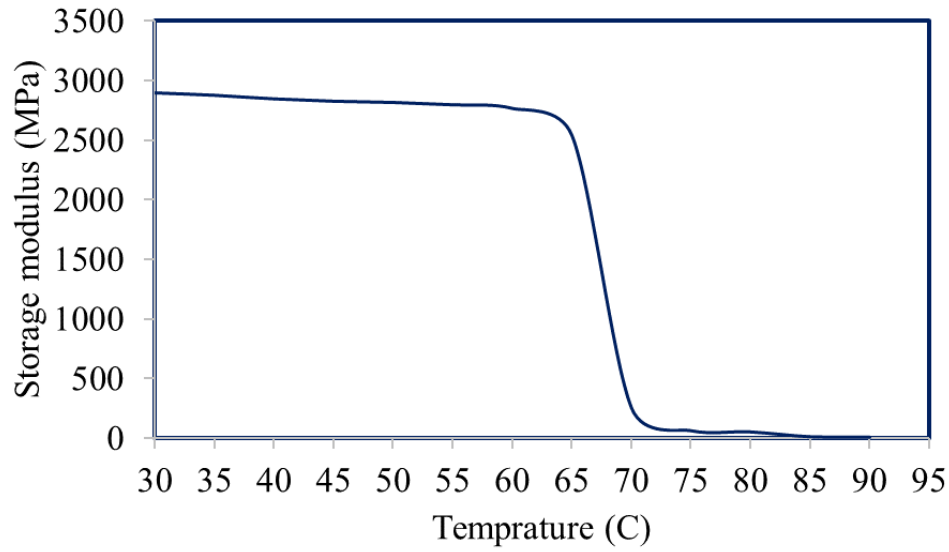


Figure 3: Dynamic Mechanical Thermal Properties of the PLA filaments

3.2 Deformation and Shape Recovery of the PLA filaments

The recovery behaviour of the PLA filament both the deformed and the recovered is shown in Table 1, Table 2, and Table 3. There was an expectation that the results would show decreasing rates of recovery as the intended test angle was increased. This expectation was due to higher forces being applied to achieve the greater angle deformations. This expectation was shown to be incorrect, as shown in Table 1 and Table 2. In fact, the results of the experiment showed no correlation between changes in the intended test angle influencing the percentage recovered. The lack of correlation would have significant implications for the future scaffold designs. The result showed that PLA polymer recover around 61.5% with SD of 4.3% regardless to the bending angle.

Table 1: Deformed PLA Test Samples































	Repeat 1	Repeat 2	Repeat 3	Repeat 4	Repeat 5
30°					
60°					
90°					
120°					
150°					
180°					

Table 2: Recovered PLA Test Samples































	Repeat 1	Repeat 2	Repeat 3	Repeat 4	Repeat 5
30°					
60°					
90°					
120°					
150°					
180°					

Table 3: The quantified results of the deformation and recovery of the PLA filaments.

Intended test angle		30	60	90	120	150	180
Repeat 1	Actual test angle	30	53	81	110	133	160
	Angle post-recovery	12	22	28	42	50	58
	Percentage recovered	60.0%	58.5%	65.4%	61.8%	62.4%	63.8%
Repeat 2	Actual test angle	31	50	80	112	131	158
	Angle post-recovery	15	22	27	32	50	66
	Percentage recovered	51.6%	56%	66.3%	71.4%	61.8%	58.2%
Repeat 3	Actual test angle	23	52	77	108	136	157
	Angle post-recovery	8	24	31	37	50	61
	Percentage recovered	65.2%	53.8%	59.7%	65.7%	63.2%	61.1%
Repeat 4	Actual test angle	30	49	79	108	137	156
	Angle post-recovery	14	18	28	40	53	60
	Percentage recovered	53.3%	63.3%	64.6%	63.0%	61.3%	61.5%
Repeat 5	Actual test angle	34	54	82	106	142	158
	Angle post-recovery	13	23	29	41	48	60
	Percentage recovered	61.8%	57.4%	64.6%	61.3%	66.2%	62.0%

3.3 Deformation and Shape Recovery of the Origami Tessellations

The two herringbone and waterbomb tessellation origami structures after twisting and recovery are shown in Figure 4. The most significant find from the measurement of the deformation and recovery of the two herringbone and Waterbomb tessellation origami structures was that the expected recovery of approximately 65.1% of each angular fold, suggested by the results of the PLA filament result, was not exhibited. The angle recovery was far greater than that shown by the filament test samples in the first experiment. Recovery rates had a mean average of 96% for the two test samples. All independent variables have been kept constant, except for the geometry of the test samples. Therefore, it can be deduced that the geometry of the origami induced internal stresses within the two models, which aided the SME and explain why such greater recovery rates were observed. The twisted waterbomb tessellation origami structures did not deform in the intended direction. The recovery of the tubular models still achieved a result that was 96% of the initial print geometry; however, because the deformation of the Waterbomb tessellation origami structure was unpredictable, it did not meet the requirements

of the biomedical scaffold, and so it was discounted as a potential biomedical scaffold to be taken forward. Only the Herringbone models were now left as the tessellation type to be taken forward, Figure 4d shows the Herringbone models after being deformed and recovered.

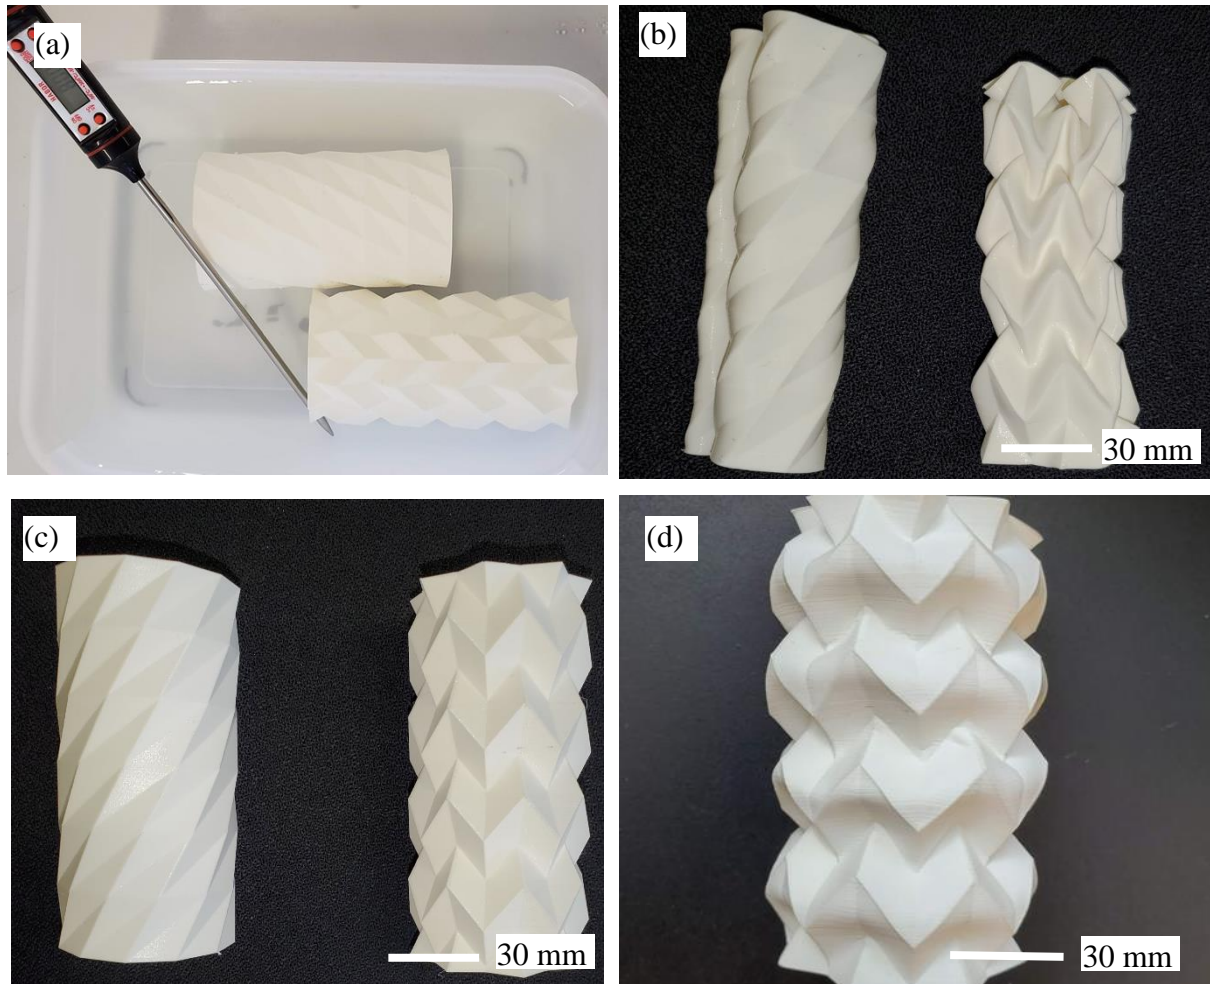


Figure 4: (a) 80°C water bath heating for waterbomb (up) and herringbone (down) tessellation origami structures (b) after deformation, (c) after recovery, (d) herringbone tessellation after being deformed and recovered for the fourth time.

To better evaluate how herringbone tessellation origami could deform and be recovered, the experiment was repeated. The difference was that this time the direction of deformation was changed from twisting to compression along the central axis. The amount of deformation observed without structural failure was far more significant. The deformation took the height from 100mm to 25mm. The recovery rate for this test was again 96%, though several cracks

were observed. This direction of deformation and recovery was repeated on the same herringbone sample several times, and the rate of recovery remained at 96% each time causing the tube to decrease in recovered height each time the test was repeated. Edges became softer each time the test was repeated, as shown in Figure 5.

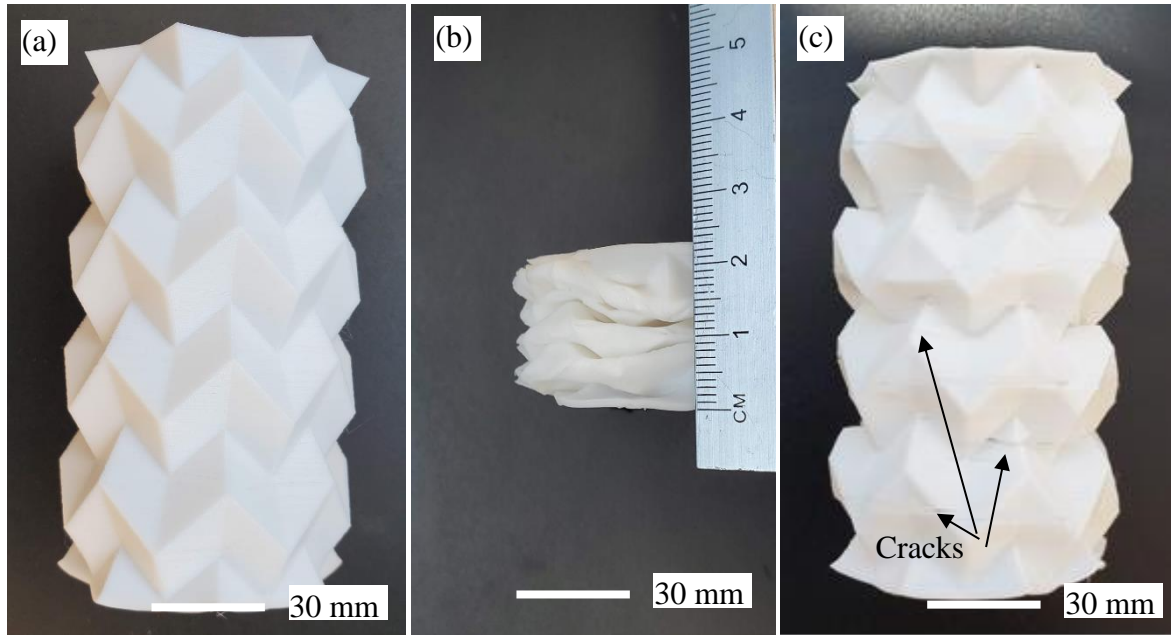


Figure 5: (a) as printed herringbone tessellation origami (b) after compression, (c) after recovery.

The scaffold interior for substituting cancellous was embedded to the herringbone tessellation origami to replicate cancellous bone and to validate its deformation and recovery behaviour. Each thin strand of the scaffold crossing the scaffold core replicates an individual trabecula. Trabeculae have a similar cross-sectional microstructure to osteons; however, Haversian canals do not pass through their centre. Therefore, the central core does not require blood vessels to pass through the replica trabeculae. The requirements of the central core's macrostructure were near enough the same as the outer compact bone substitute section of the scaffold. The only real difference being the density of the central core needed to be less to create the large pores visible in cancellous bone. The herringbone tessellation origami was combined with the central

core to create the final CAD model, shown in Figure 6a. Figure 6b shows the 3D printed sample with the porous central core. The figure shows core how light can pass through the cancellous scaffold substitute, proving that the pores are interconnected

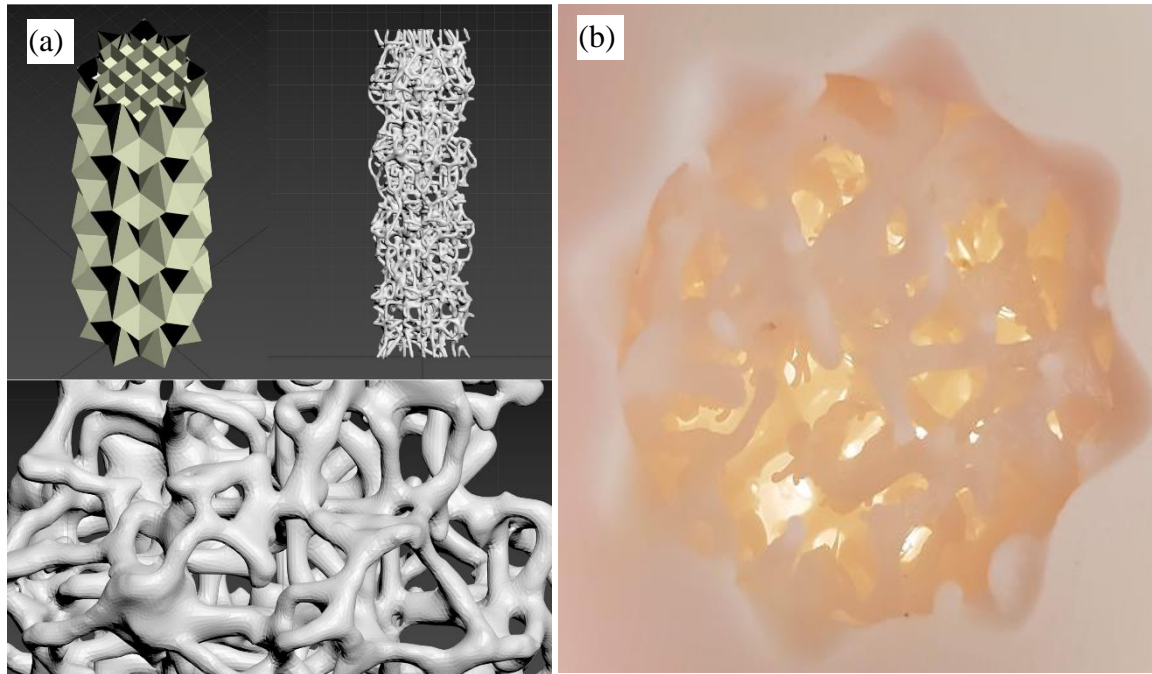


Figure 6: (a) design of the central core, (b) 3D printed of herringbone tessellation origami with substituting cancellous core.

The same SME procedure was applied to the process herringbone tessellation origami with substituting cancellous core, and the results are shown in Figure 7. Unsurprisingly the amount that the model deformed was considerably less than the tubular prototypes shown in Figure 5 due to the substantial increase in stiffness of the central core. Despite this, the scaffold was deformed to 70mm and then recovered to 95mm, as shown in Figure 7. All previous experiments had been testing individual aspects of the developed design to optimise the SME for when combined into the final design. Therefore, this was the first test exploring how the SME of a full scaffold prototype, and it was relatively successful, though the deformation was less than the tubular models. Future investigations will consider the effect of parameters such as layer thickness and building directions on the SME.

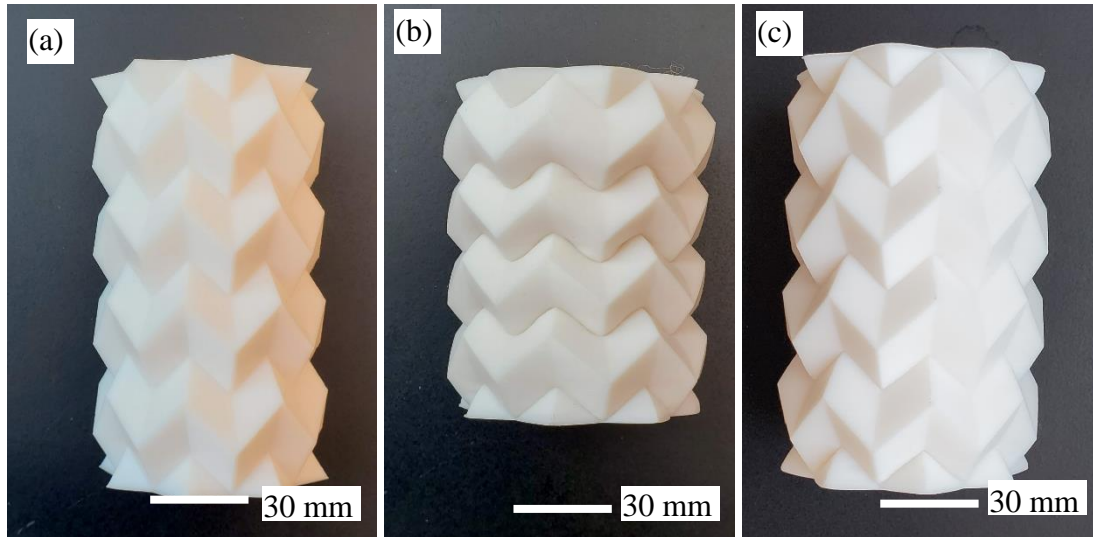


Figure 7: (a) as printed herringbone tessellation origami with porous core (b) after compression, (c) after recovery.

4. Conclusions

A novel concept of deployable scaffolds using a combination of origami and 4D printing technologies was introduced. The design strategy applied in the paper is based on the creation of porous origami structures in its nearly final shape and deformed into a volume suitable for minimal invasion surgeries. We characterised the shape memory behaviour of the PLA material and the manufactured designs. We characterised the shape memory behaviour of the PLA filaments and the manufactured designs. The PLA filaments showed a constant shape recovery of about 61% regardless of the deformation amount. On the other hand, Tubular herringbone tessellation origami showed significant deformation capabilities and a high recovery rate of about 96% despite the presence of cracks in the deformed samples. The same recovery rate was achieved when adding porous natural cancellous bone core to the herringbone tessellation origami though the deformation amount was less significant. Future studies are recommended to characterise the mechanical and biocompatible properties that are needed for the clinical adoption of this approach. The use of 4D printing in situ with origami structures is relatively

inexpensive and easy to implement which makes it also suitable for the development of a wide range of foldable structures.

References

1. D. Lacroix: ‘4 - Biomechanical aspects of bone repair’, in ‘Bone Repair Biomaterials’, (eds. J. A. Planell, et al.), 106-118; 2009, Woodhead Publishing.
2. K. Hasegawa, C. H. Turner, and D. B. Burr, *Calcified Tissue International*, 1994, **55**(5), 381-386.
3. M. Elsayed, M. Ghazy, Y. Youssef, and K. Essa, *Rapid Prototyping Journal*, 2019, **25**(3), 433-447.
4. K. Essa, H. Hassanin, M. M. Attallah, N. J. Adkins, A. J. Musker, G. T. Roberts, N. Tenev, and M. Smith, *Applied Catalysis A: General*, 2017, **542**, 125-135.
5. T. D. Ngo, A. Kashani, G. Imbalzano, K. T. Q. Nguyen, and D. Hui, *Composites Part B: Engineering*, 2018, **143**, 172-196.
6. L. Chaunier, S. Guessasma, S. Belhabib, G. Della Valle, D. Lourdin, and E. Leroy, *Additive Manufacturing*, 2018, **21**, 220-233.
7. W. Liu, H. Wu, Z. Tian, Y. Li, Z. Zhao, M. Huang, X. Deng, Z. Xie, and S. Wu, *Journal of the American Ceramic Society*, 2019, **102**(5), 2257-2262.
8. X. Zheng, H. Lee, T. Weisgraber, M. Shusteff, J. DeOtte, E. Duoss, J. Kuntz, M. Biener, Q. Ge, J. Jackson, S. Kucheyev, N. Fang, and C. Spadaccini, *Science*, 2014, **344**, 1373-1377.
9. Y.-M. Ha, J.-W. Choi, and S. Lee, *Journal of Mechanical Science and Technology*, 2008, **22**, 514-521.
10. E. Behroodi, H. Latifi, and F. Najafi, *Scientific Reports*, 2019, **9**(1), 19692.
11. H. Hassanin and K. Jiang, *Microelectronic Engineering*, 2011, **88**(11), 3275-3277.
12. H. Hassanin and K. Jiang, *Journal of Micromechanics and Microengineering*, 2013, **24**(1), 015018.
13. H. Hassanin and K. Jiang, *Scripta Materialia*, 2013, **69**(6), 433-436.
14. H. Hassanin and K. Jiang, *Microelectronic Engineering*, 2010, **87**(5), 1610-1613.
15. H. Hassanin and K. Jiang, *Microelectronic Engineering*, 2009, **86**(4), 929-932.
16. H. Hassanin and K. Jiang, *Advanced Engineering Materials*, 2009, **11**(1 - 2), 101-105.
17. H. Hassanin and K. Jiang, *Microelectronic Engineering*, 2010, **87**(5), 1617-1619.
18. L. E. Murr, *Journal of Materials Research and Technology*, 2020, **9**(1), 1087-1103.
19. C. A. Chatham, T. E. Long, and C. B. Williams, *Progress in Polymer Science*, 2019, **93**, 68-95.
20. S. Bose, D. Banerjee, A. Shivaram, S. Tarafder, and A. Bandyopadhyay, *Materials and Design*, 2018, **151**, 102-112.
21. A. Shivaram, S. Bose, and A. Bandyopadhyay, *Acta Biomaterialia*, 2017, **58**, 550-560.
22. V. K. Balla, M. Das, S. Bose, G. D. Janaki Ram, and I. Manna, *Materials Science and Engineering C*, 2013, **33**(8), 4594-4598.
23. A. Mostafaei, A. M. Elliott, J. E. Barnes, F. Li, W. Tan, C. L. Cramer, P. Nandwana, and M. Chmielus, *Progress in Materials Science*, 2020, 100707.
24. M. Ziaee and N. B. Crane, *Additive Manufacturing*, 2019, **28**, 781-801.

25. X. Lv, F. Ye, L. Cheng, S. Fan, and Y. Liu, *Ceramics International*, 2019, **45**(10), 12609-12624.
26. Y. Zhang, W. Jarosinski, Y.-G. Jung, and J. Zhang: '2 - Additive manufacturing processes and equipment', in 'Additive Manufacturing', (eds. J. Zhang, et al.), 39-51; 2018, Butterworth-Heinemann.
27. A. Mohammed, A. Elshaer, P. Sareh, M. Elsayed, and H. Hassanin, *International Journal of Pharmaceutics*, 2020, **580**, 119245.
28. J. Goole and K. Amighi, *International Journal of Pharmaceutics*, 2016, **499**(1), 376-394.
29. B. Derby, *Engineering*, 2015, **1**(1), 113-123.
30. B. Derby: 'Inkjet Printing of Functional and Structural Materials: Fluid Property Requirements, Feature Stability, and Resolution', in 395-414; 2010.
31. C. Qiu, N. J. E. Adkins, H. Hassanin, M. M. Attallah, and K. Essa, *Materials & Design*, 2015, **87**, 845-853.
32. H. Klippstein, H. Hassanin, A. Diaz De Cerio Sanchez, Y. Zweiri, and L. Seneviratne, *Advanced Engineering Materials*, 2018, **20**(9), 1800290.
33. Essa, K.; Khan, R.; Hassanin, H.; Attallah, M.M.; Reed, R. An iterative approach of hot isostatic pressing tooling design for net-shape IN718 superalloy parts. *Int. J. Adv. Manuf. Technol.* 2016, **83**, 1835–1845.
34. A. Galatas, H. Hassanin, Y. Zweiri, and L. Seneviratne, *Polymers*, 2018, **10**(11), 1262.
35. H. Hassanin, L. Finet, S. C. Cox, P. Jamshidi, L. M. Grover, D. E. T. Shepherd, O. Addison, and M. M. Attallah, *Additive Manufacturing*, 2018, **20**, 144-155.
36. S. Li, H. Hassanin, M. M. Attallah, N. J. E. Adkins, and K. Essa, *Acta Materialia*, 2016, **105**, 75-83.
37. A. Sabouri, A. K. Yetisen, R. Sadigzade, H. Hassanin, K. Essa, and H. Butt, *Energy & Fuels*, 2017, **31**(3), 2524-2529.
38. A. Lendlein and S. Kelch, *Angewandte Chemie International Edition*, 2002, **41**(12), 2034-2057.
39. J. Xu and J. Song: '10 - Polylactic acid (PLA)-based shape-memory materials for biomedical applications', in 'Shape Memory Polymers for Biomedical Applications', (ed. L. H. Yahia), 197-217; 2015, Woodhead Publishing.
40. R. Pawar, S. Tekale, S. Shisodia, J. Totre, and A. Domb, *Recent Patents on Regenerative Medicine*, 2014, **4**.
41. Y. Chen, J. Yan, and J. Feng, *Symmetry*, 2019, **11**(9).
42. N. Uomini and R. Lawson, *Symmetry*, 2017, **9**(9).